

# Spinal stabilization implant


ennoia<sup>vet</sup>

Personalized Engineering for Surgery



## USE OF THE DEVICE

Vertebral instability with or without dislocation

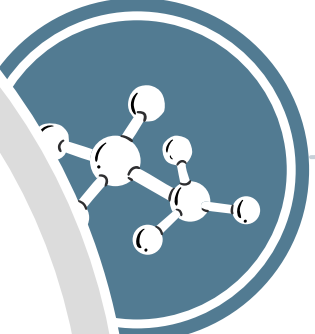

## MATERIAL

Titanium




## STERILISATION

Autoclavable device



## COMPLETION TIME

5 weeks

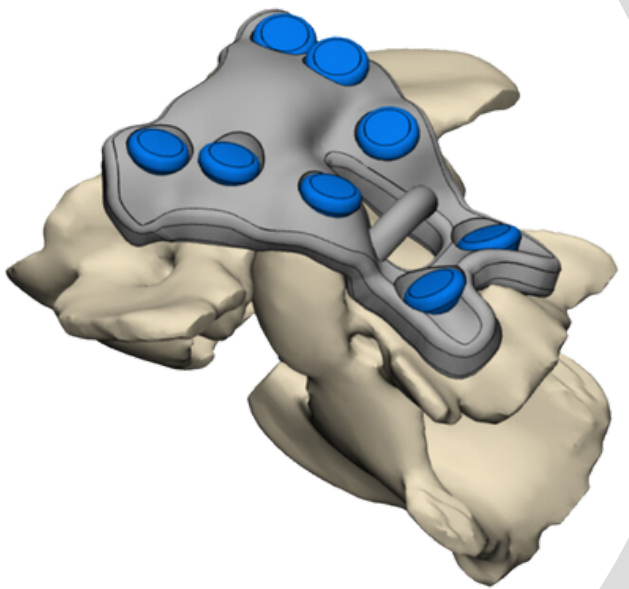

ennoia offers spinal stabilization implants to perform arthrodesis.

The implants are combined with drilling guides to have a precise position of the screws in the vertebral bodies.

Single-use product for a single patient.